

Experimental paper

Hemodynamic improvement of a LUCAS 2 automated device by addition of an impedance threshold device in a pig model of cardiac arrest[☆]



Guillaume Debaty^{a,b}, Nicolas Segal^c, Tim Matsuura^d, Brian Fahey^a, Marvin Wayne^e, Brian Mahoney^f, Ralph Frascione^g, Charles Lick^h, Demetris Yannopoulos^{a,*}

^a Department of Medicine–Cardiovascular Division, University of Minnesota, Minneapolis, MN, United States

^b UJF–Grenoble 1/CNRS/CHU de Grenoble/TIMC-IMAG UMR 5525, Grenoble, France

^c AP-HP, Hôpital Lariboisière, Services des Urgences, Univ Paris Diderot, Sorbonne Paris Cité, UMRS 942, F-75018 Paris, France

^d Department of Integrated Biology & Physiology, Medical School, University of Minnesota, Minneapolis, MN, United States

^e Whatcom County Emergency Medical Services, Department of Emergency Medicine, PeaceHealth St. Joseph Medical Center, Bellingham, WA, United States

^f Department of Emergency Medicine, Hennepin County Medical Center, Minneapolis, MN, United States

^g Department of Emergency Medicine, Regions Hospital, St. Paul, MN, United States

^h Allina Health Emergency Medical Services, St. Paul, MN, United States

ARTICLE INFO

Article history:

Received 7 July 2014

Received in revised form 23 August 2014

Accepted 8 September 2014

Keywords:

Cardiac arrest

Cardiopulmonary resuscitation (CPR)

Mechanical CPR

Impedance threshold device

ABSTRACT

Introduction: The combination of the LUCAS 2 (L-CPR) automated CPR device and an impedance threshold device (ITD) has been widely implemented in the clinical field. This animal study tested the hypothesis that the addition of an ITD on L-CPR would enhance cerebral and coronary perfusion pressures.

Methods: Ten female pigs (39.0 ± 2.0 kg) were sedated, intubated, anesthetized with isoflurane, and paralyzed with succinylcholine (93.3 μg/kg/min) to inhibit the potential confounding effect of gasping. After 4 min of untreated ventricular fibrillation, 4 min of L-CPR + an active ITD or L-CPR + a sham ITD was initiated and followed by another 4 min of the alternative method of CPR. Systolic blood pressure (SBP), diastolic blood pressure (DBP), diastolic right atrial pressure (RAP), intracranial pressure (ICP), airway pressure, and end tidal CO₂ (ETCO₂) were recorded continuously. Data expressed as mean mmHg ± SD.

Results: Decompression phase airway pressure was significantly lower with L-CPR + active ITD versus L-CPR + sham ITD (−5.3 ± 2.2 vs. −0.5 ± 0.6; $p < 0.001$). L-CPR + active ITD treatment resulted in significantly improved hemodynamics versus L-CPR + sham ITD: ETCO₂, 35 ± 6 vs. 29 ± 7 ($p = 0.015$); SBP, 99 ± 9 vs. 93 ± 15 ($p = 0.050$); DBP, 24 ± 12 vs. 19 ± 15 ($p = 0.006$); coronary perfusion pressure, 29 ± 8 vs. 26 ± 7 ($p = 0.004$) and cerebral perfusion pressure, 24 ± 13 vs. 21 ± 12 ($p = 0.028$).

Conclusions: In pigs undergoing L-CPR the addition of the active ITD significantly reduced intrathoracic pressure and increased vital organ perfusion pressures.

© 2014 Elsevier Ireland Ltd. All rights reserved.

1. Introduction

Quality of cardiopulmonary resuscitation (CPR) is critical to improving survival rates with favorable neurological function.¹ Even when optimally performed, blood flow generated by

manual chest compressions is, at best, less than 25% of normal.^{2,3} Mechanical chest compression devices have been developed to improve the quality of CPR by replacing manual compressions. The LUCAS device consistently compresses the chest at a rate of 100/min and a depth of 5 cm and provides three pounds of upward force with each decompression. Animal studies with the Lund University Cardiopulmonary Assist System (LUCAS) have shown improved organ perfusion pressures, enhanced cerebral blood flow, and higher end-tidal CO₂ during CPR compared with the use of manual compressions.^{4–6}

Similarly, the impedance threshold device (ITD) has also been shown to improve overall CPR hemodynamics including cerebral and coronary perfusion pressure. It works by impeding inflow

[☆] A Spanish translated version of the summary of this article appears as Appendix in the final online version at <http://dx.doi.org/10.1016/j.resuscitation.2014.09.013>.

* Corresponding author at: Department of Internal Medicine, Division of Cardiology, University of Minnesota, 420 Delaware Street S.E., MMC 508, Minneapolis, MN 55455, United States.

E-mail address: yanno001@umn.edu (D. Yannopoulos).

of respiratory gases during the decompression phase of CPR, thereby generating a greater negative intrathoracic pressure with each chest recoil. This, in turn, enhances venous return and lowers intracranial pressure thereby enhancing cardiac and cerebral perfusion^{7,8}.

As in the case of standard manual CPR, we hypothesize that when an active ITD is added on L-CPR, cerebral and coronary perfusion pressures will improve.

2. Methods

This study was approved by the Institutional Animal Care Committee of the Minneapolis Medical Research Foundation of Hennepin County Medical Center. All animal care was compliant with the National Research Council's 1996 Guidelines for the Care and Use of Laboratory Animals. All studies were performed by a qualified, experienced research team in Yorkshire female farm bred pigs weighing 39 ± 2 kg. A certified and licensed veterinarian assured the protocols were performed in accordance with the National Research Council's guidelines.

2.1. Preparatory phase

The surgical preparation, anesthesia, data monitoring, and recording procedures used in this study have been previously described.⁹ Under aseptic surgical conditions, we used initial sedation with intramuscular ketamine (10 mL of 100 mg/mL, Ketaset, Fort Dodge Animal Health, Fort Dodge, Iowa) followed by inhaled isoflurane at a dose of 0.8–1.2%. Pigs were intubated with a size of 7.0 endotracheal tube. The animal's temperature was maintained at normothermia, with a warming blanket (Bair Hugger, Augustine Medical, Eden Prairie, Minnesota). Central aortic blood pressure was recorded continuously with a micromanometer-tipped catheter (Mikro-Tip Transducer, Millar Instruments, Houston, TX) placed in the descending thoracic aorta via the femoral artery using a modify Seldinger technique. A second Millar catheter was inserted in the right atrium via the right external jugular vein. An ultrasound flow probe (Transonic 420 series multichannel, Transonic Systems, Ithaca, NY) was placed in the left common carotid artery to quantify carotid blood flow (mL/min). After creating a burr hole, an intracranial bolt was positioned at the right parietal aspect of the cranium. A Millar catheter was then inserted into the parietal lobe to measure intracranial pressure (ICP).

In addition to isoflurane and ketamine, all animals received an intravenous heparin bolus (100 units/kg), an infusion of succinylcholine (93.3 μ g/kg/min), and an infusion of 1 L of saline. All animals were ventilated with room air using a volume-control ventilator (Narcomed, Telford, Pennsylvania), a tidal volume of 10 mL/kg and a respiratory rate adjusted to continually maintain a PaCO₂ between 38 and 42 mmHg and PaO₂ around 80 mmHg (blood oxygen saturation >95%), as measured from arterial blood gas (Gem 3000, Instrumentation Laboratory). Surface electrocardiographic tracings were continuously recorded. All data were recorded with a digital recording system (BIOPAC MP 150, BIOPAC Systems, Inc., CA, USA). End tidal CO₂ (ETCO₂), tidal volume, minute ventilation, and blood oxygen saturation were continuously measured with a respiratory monitor (Cosmo Plus, Novamatrix Medical Systems, Wallingford, CT).

2.2. Measurements and recording

Aortic pressure, right atrial pressure, ICP, ETCO₂, and carotid blood flow were continuously recorded. Coronary perfusion pressure (CPP) was calculated as the difference between right atrial pressure and diastolic aortic pressure during the decompression

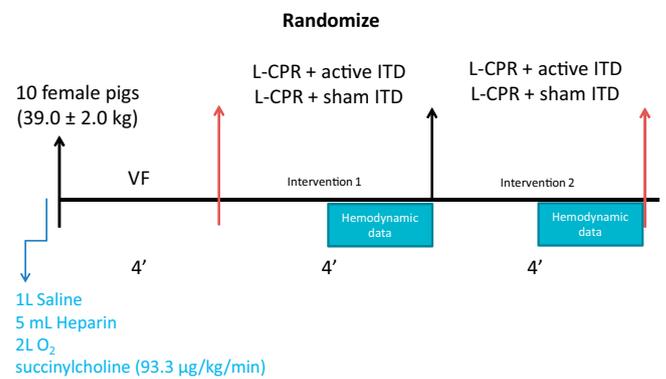


Fig. 1. Study protocol.

phase of CPR. Cerebral perfusion pressure (CePP) was calculated as the difference between mean aortic pressure and mean ICP. Ultrasound-derived carotid blood flow was reported in mL/min.

2.3. Experimental protocol

After the surgical preparation was complete, oxygen saturation on room air was greater than 95%, and ETCO₂ was stable between 38 and 42 mmHg for 5 min, ventricular fibrillation was induced by direct intracardiac current via a temporary pacing wire. The ventilator was disconnected from the endotracheal tube. As described below in the protocol mechanical CPR was performed using the LUCAS 2™ (Physio-Control, Redmond, WA) compression system at a rate of 100 compressions/min with a 50% duty cycle. According to randomization order, either an impedance threshold device with a resistance of 16 cmH₂O (ITD, ResQPOD™, Advanced Circulatory Systems, Roseville, MN) or a sham ITD with no inspiratory resistance was attached to the endotracheal tube. Asynchronous positive pressure ventilations were delivered with 2 L/min of O₂ with a manual resuscitator bag. The tidal volume was maintained at 10 mL/kg determined by measuring the inspiratory tidal volume using the Cosmo Plus described above, and the respiratory rate was 10 breaths/min.

The protocol was as follows: after 4 min of untreated ventricular fibrillation, 10 pigs were block randomized on a crossover design to receive either L-CPR + active ITD for 4 min then L-CPR + sham ITD for 4 min or to the same interventions in reverse order (Fig. 1). Hemodynamic data were recorded continuously during the protocol and specific data elements were analyzed during the final 2 min of each intervention to allow for the animal to stabilize after the change of CPR method. Arterial blood gas samples were collected during the baseline and then after 3.5 min of CPR during each intervention. After 8 min of CPR, animals were sacrificed with a 10 mL injection of 10 M potassium chloride.

2.4. Statistical analysis

Data are expressed as mean \pm standard deviation (SD). Mean values were compared with the Student's paired *t* test. To assess for the potential of a carry-over effect based upon randomization order a Student unpaired *t* test was performed comparing mean CPP and CePP values during the first intervention period versus the second period. Normality of data was tested using the Kolmogorov Smirnov test. All statistical tests were two-sided, and a *p* value of less than 0.05 was required to reject the null hypothesis. Statistical analysis was performed using IBM SPSS Statistics 21.

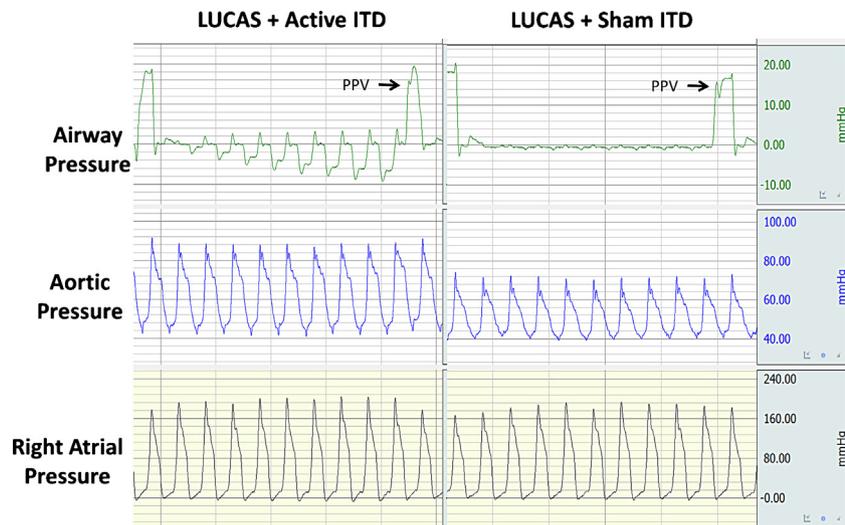


Fig. 2. Example of pressure recording with the 2 interventions. Airway pressure was measured as a surrogate for intrathoracic pressure. Pressures expressed in mmHg. PPV, positive pressure ventilation.

3. Results

There were no statistical differences in baseline characteristics, regardless of the randomization order. Further, there was no evidence of a carryover effect based on the randomization order for the primary study endpoints (mean CPP of the 1st period vs. the 2nd was 29 ± 8 vs. 27 ± 8 , $p = 0.71$ and CePP was 23 ± 11 vs. 22 ± 14 , $p = 0.48$).

3.1. Airway pressure

During CPR, airway pressure, a surrogate for intrathoracic pressure, was significantly lower during decompression in the active ITD group (-5.3 ± 2.2 mmHg vs. -0.5 ± 0.6 , $p < 0.005$). During the compression phase of CPR, airway pressure was higher in the active ITD group (2.9 ± 1.4 mmHg vs. 0.9 ± 0.7 , $p = 0.006$). Representative airway pressure curves are shown in Fig. 2.

3.2. Hemodynamics

L-CPR+active ITD treatment resulted in a significant increase in systolic and diastolic blood pressure, CePP and CPP versus L-CPR+sham ITD (Table 1). The CePP and CPP were consistently increased with use of the active ITD versus the sham device over time.

Table 1
Comparison of mean hemodynamic results.

	LUCAS + sham ITD	LUCAS + active ITD	<i>p</i>
Systolic blood pressure	92 ± 15	99 ± 9	0.041
Diastolic blood pressure	35 ± 7	38 ± 8	0.005
Carotid blood flow (mL/min)	85 ± 28	80 ± 17	0.65
Intracranial pressure	30 ± 9	31 ± 11	0.26
End tidal CO ₂ (mmHg)	29 ± 7	35 ± 6	0.012
Coronary perfusion pressure	26 ± 7	29 ± 8	0.009
Cerebral perfusion pressure	21 ± 12	24 ± 13	0.021

Values are shown as mean \pm SD. All pressures in mmHg.

3.3. Blood gas

There were no statistically significant differences regarding pH, PCO₂ and PO₂ within the different interventions (Table 2).

4. Discussion

The results demonstrated that the application of negative intrathoracic pressure during CPR with the combination of an ITD and the LUCAS 2 mechanical CPR device increased vital organ perfusion pressures during cardiac arrest resuscitation. The beneficial effect of the ITD was consistent over the duration of L-CPR. To our knowledge this study is the first to assess the beneficial effect on hemodynamics with this device combination.

In animal and human studies, the addition of an ITD to standard and active compression decompression CPR (ACD-CPR) has been shown to improve hemodynamics, carotid blood flow (a surrogate of cerebral blood flow), and myocardial and cerebral perfusion.^{10–12} Previous studies in pigs have shown that the ITD decreases intrathoracic pressure in the range of -4 to -8 mmHg during CPR.^{8,10} The results from the current study were consistent with these prior observations both in terms of the decrease in airway pressures and the improvement in hemodynamics. The findings in the current study demonstrate that it is possible to augment circulation with high quality compressions, active decompression with up to three pounds of decompression force and an active ITD. These observations are supportive of, and consistent with, recent studies that have demonstrated that optimal clinical outcomes with standard CPR by itself, or standard CPR and the active ITD, require high quality CPR.^{13–15}

This study has several limitations. First, we chose to randomize the two interventions consecutively on the same animals to reduce

Table 2
Arterial blood gas analysis.

	Baseline	LUCAS + sham ITD	LUCAS + active ITD	<i>p</i>
pH	7.44 ± 0.03	7.33 ± 0.05	7.31 ± 0.06	0.31
PO ₂	204 ± 114	121 ± 87	109 ± 73	0.16
PCO ₂	45 ± 2.9	47 ± 6.5	50 ± 6.4	0.60

Values are shown as mean \pm SD. All pressures are in mmHg, *p* values are calculated between the 2 treatments group.

inter-animal variability. Although the effects of CPR can change over time the relatively short untreated ventricular fibrillation time interval was not anticipated to impact the assessment of the active ITD. This assumption appears to have been correct. Secondly, the results of this study demonstrate a significant albeit modest increase in ETCO₂, CePP and CPP with L-CPR+ active ITD however we did not measure actual vital organ blood flow. Nonetheless, prior studies have shown a significant correlation between organ perfusion, ETCO₂, CePP and CPP.¹¹

5. Conclusion

In pigs undergoing L-CPR the addition of the ITD significantly reduced intrathoracic pressure and improved both coronary and cerebral perfusion pressures. This hemodynamic benefit warrants further study in longer term outcomes.

Funding

This study was funded by an internal grant of the Cardiovascular Division of the University of Minnesota.

Conflict of interest statement

The authors have no financial conflicts of interest.

Appendix A. Supplementary data

Supplementary data associated with this article can be found, in the online version, at <http://dx.doi.org/10.1016/j.resuscitation.2014.09.013>.

References

1. Meaney PA, Bobrow BJ, Mancini ME, et al. Cardiopulmonary resuscitation quality: improving cardiac resuscitation outcomes both inside and outside the hospital: a consensus statement from the American Heart Association. *Circulation* 2013;128:417–35.
2. Cohen TJ, Tucker KJ, Lurie KG, et al. Active compression–decompression. A new method of cardiopulmonary resuscitation. *Cardiopulmonary Resuscitation Working Group. J Am Med Assoc* 1992;267:2916–23.
3. Duggal C, Weil MH, Gazmuri RJ, et al. Regional blood flow during closed-chest cardiac resuscitation in rats. *J Appl Physiol* 1993;74:147–52.
4. Steen S, Liao Q, Pierre L, Paskevicius A, Sjoberg T. Evaluation of LUCAS, a new device for automatic mechanical compression and active decompression resuscitation. *Resuscitation* 2002;55:285–99.
5. Rubertsson S, Karlsten R. Increased cortical cerebral blood flow with LUCAS: a new device for mechanical chest compressions compared to standard external compressions during experimental cardiopulmonary resuscitation. *Resuscitation* 2005;65:357–63.
6. Axelsson C, Karlsson T, Axelsson AB, Herlitz J. Mechanical active compression–decompression cardiopulmonary resuscitation (ACD-CPR) versus manual CPR according to pressure of end tidal carbon dioxide (P(ET)CO₂) during CPR in out-of-hospital cardiac arrest (OHCA). *Resuscitation* 2009;80:1099–103.
7. Lurie KG, Coffeen P, Shultz J, McKnite S, Detloff B, Mulligan K. Improving active compression–decompression cardiopulmonary resuscitation with an inspiratory impedance valve. *Circulation* 1995;91:1629–32.
8. Lurie KG, Zielinski T, McKnite S, Aufderheide T, Voelckel W. Use of an inspiratory impedance valve improves neurologically intact survival in a porcine model of ventricular fibrillation. *Circulation* 2002;105:124–9.
9. Lurie KG, Yannopoulos D, McKnite SH, et al. Comparison of a 10-breaths-per-minute versus a 2-breaths-per-minute strategy during cardiopulmonary resuscitation in a porcine model of cardiac arrest. *Respir Care* 2008;53:862–70.
10. Lurie KG, Mulligan KA, McKnite S, Detloff B, Lindstrom P, Lindner KH. Optimizing standard cardiopulmonary resuscitation with an inspiratory impedance threshold valve. *Chest* 1998;113:1084–90.
11. Lurie KG, Voelckel WG, Zielinski T, et al. Improving standard cardiopulmonary resuscitation with an inspiratory impedance threshold valve in a porcine model of cardiac arrest. *Anesth Analg* 2001;93:649–55.
12. Pirralo RG, Aufderheide TP, Provo TA, Lurie KG. Effect of an inspiratory impedance threshold device on hemodynamics during conventional manual cardiopulmonary resuscitation. *Resuscitation* 2005;66:13–20.
13. Stiell IG, Brown SP, Christenson J, et al. What is the role of chest compression depth during out-of-hospital cardiac arrest resuscitation. *Crit Care Med* 2012;40:1192–8.
14. Abella BS, Sandbo N, Vassilatos P, et al. Chest compression rates during cardiopulmonary resuscitation are suboptimal: a prospective study during in-hospital cardiac arrest. *Circulation* 2005;111:428–34.
15. Idris AH, Guffey D, Pepe PE, et al. The interaction of chest compression rates with the impedance threshold device and association with survival following out-of-hospital cardiac arrest – abstract late breaking clinical trial. *Circulation* 2012;126:2776–99.